TEQAS Evaluation

todylaboratories
EQA Schemes

CUSTOMER CODE 9593/TQC316-14


Coagulation 05/2016 Sample CO0216 TQCO0023-May-2016

APTT (s)

Instrument
Reagent APTT - Technoclone (own group)
Method: Siron LS

Observations APTT Liquid


Distribution of the results

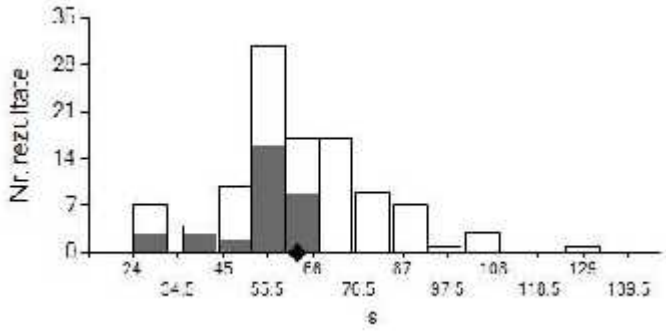

Own results 62,30 s

History of the results

Month	Sample Code	X (Mean)	Result	Bias (Diff%)
5/2016	CO0216	55,47	62,30	12,31
3/2016	CO0116	27,26	26,30	-3,53
11/2015	CO0415	33,92	44,20	30,30
9/2015	CO0315	25,73	27,30	6,10
5/2015	CO0215	25,68	26,10	1,65
3/2015	CO0115	31,48	33,40	6,10
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

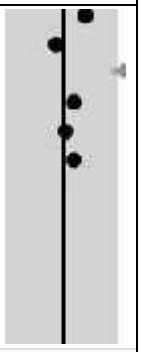

-30% x +30%

Results	x (mean)	SD (standard deviation)	CV%	n(no. of results)	x±30%(target-limit)	Z Score
Own group	55,47	5,91	10,65	33	38,83 - 72,11	1,16
All methods	62,57	17,30	27,65	107	43,80 - 81,34	-0,02